

## CATPHAN Low Contrast - 515 Module Report

### OVERALL RESULTS



ALL TOLERANCES PASSING




ANALYSIS COMPLETE

### Image Information

Filename	C:\RIT\RIT113V4\Demo Images\Radia Demo Images\CATPHAN\CTP515
Institution	Chlidrens Hospital
Station	CTER_OC0
kVp	140
mA	400
Protocol	1.1 Physics Test
Filter	
Convolution Kernel	STANDARD
DICOM Slice Thickness(mm)	5
SOP Instance UID	1.2.840.113619.2.55.3.51037702.5388.1181828433.292.16
Slice Location	0

### Analysis Image

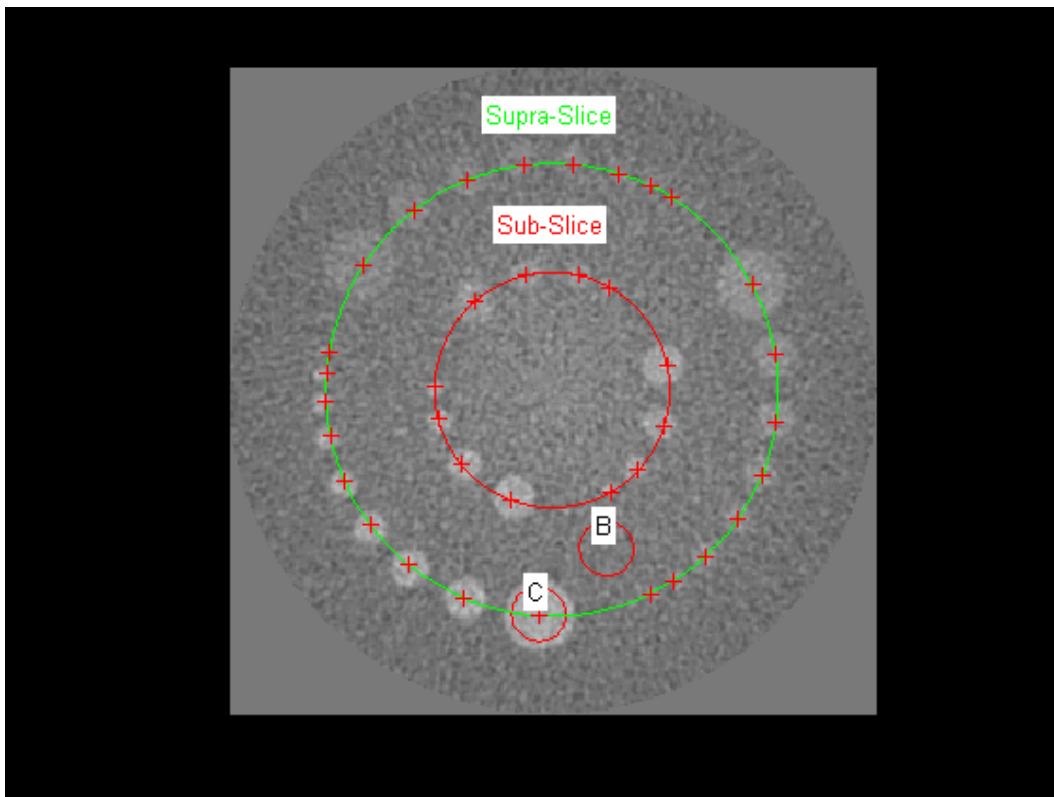

## Detected Targets

Band	Number of Objects Detected (Nominal)	Pass/Fail
Subslice	12 of 12 (10)	Pass
Supraslice	25 of 27 (23)	Pass

## Contrast to Noise Ratio

CNR	Minimum CNR	Pass/Fail
4.04	2	Pass

## Analysis Settings

Trim Margin	0
-------------	---