

ACR MR Phantom - Localizer Report

OVERALL RESULTS



ALL TOLERANCES PASSING




ANALYSIS COMPLETE

Image Information

Filename	C:\RIT\RIT113V4\demo images_old\Radia Demo Images\ACR_MRI\Localizer.dcm
Institution	Rocky Mountain Open Scan-Golden
Station	MRC17485
Magnetic Field Strength	1.494
Protocol	Sagittal_Localizer
DICOM Slice Thickness(mm)	20
SOP Instance UID	1.3.12.2.1107.5.2.6.23452.30000007020103405234300001227
Slice Location	0
Echo Time	20
Repetition Time	200
In Plane Phase Encoding Direction	ROW
Pixel Bandwidth	400
ReceiveCoilName	
Transmit Coil Name	Body
Flip Angle	90
Device Serial Number	23452
Software Version	syngo MR 2004A 4VA25A
Scan Options	
Echo Number	0
Echo Train Length	1
Operating Mode	

Analysis Image

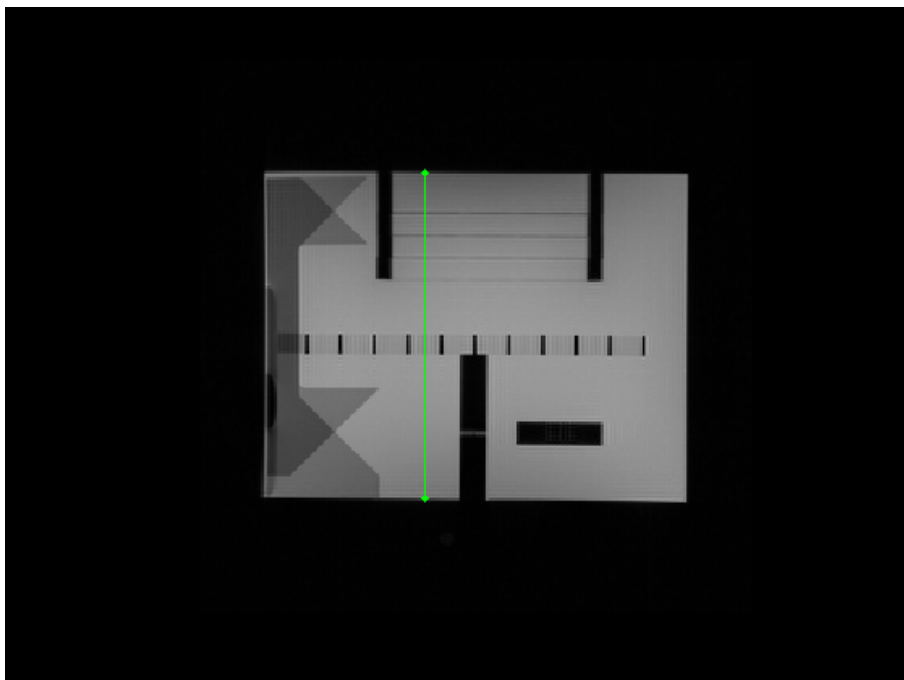

Localizer Line Length

Localizer Line Length (mm)	148.01
ACR Minimum (mm)	143.00
ACR Maximum (mm)	153.00
Pass-Fail	Pass

Analysis Settings

Localizer Phantom Threshold	0.5
-----------------------------	-----