


Rapid ARC Test 2 Report

Dose Rate Image



Open Field Image

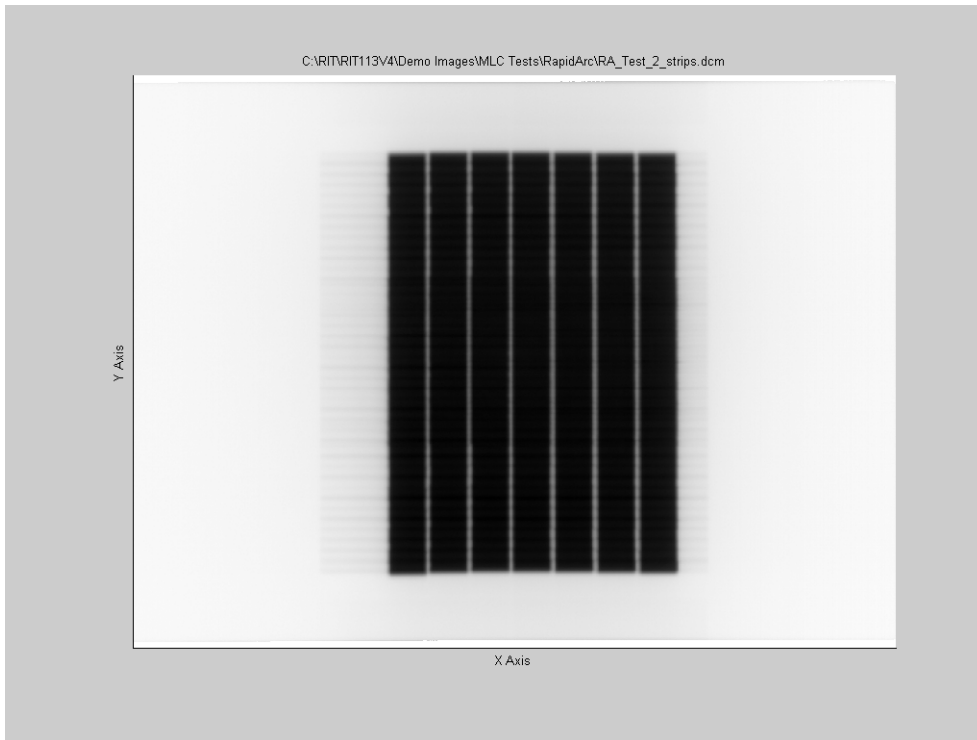

Area Statistics

	F1	F2	F3	F4	F5	F6	F7
Leaf 1 Corr. Reading	152.3257	153.3494	153.7923	154.0106	154.0107	153.7739	152.7048
Leaf 1 Deviation(%)	-0.71578	-0.04857	0.24008	0.38242	0.38243	0.22813	-0.4687
Leaf 1 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 2 Corr. Reading	152.8744	153.9973	154.4502	154.7107	154.6769	154.4388	153.2956
Leaf 2 Deviation(%)	-0.77176	-0.042933	0.25105	0.42013	0.39823	0.24368	-0.49839
Leaf 2 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 3 Corr. Reading	153.1699	154.4257	155.0129	155.2728	155.1775	154.834	153.6328
Leaf 3 Deviation(%)	-0.86326	-0.05047	0.32959	0.49783	0.43617	0.2138	-0.56366
Leaf 3 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 4 Corr. Reading	153.432	154.8078	155.2201	155.5017	155.5731	155.1537	153.8414
Leaf 4 Deviation(%)	-0.87728	0.011505	0.27788	0.45978	0.50594	0.23498	-0.61281
Leaf 4 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 5 Corr. Reading	153.5707	154.8635	155.386	155.6763	155.7013	155.3684	154.0224
Leaf 5 Deviation(%)	-0.88455	-0.05018	0.2871	0.47441	0.49054	0.27569	-0.59301
Leaf 5 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 6 Corr. Reading	153.7677	155.0201	155.6055	155.9132	155.8539	155.6144	154.105
Leaf 6 Deviation(%)	-0.87539	-0.06807	0.30931	0.50767	0.46945	0.31501	-0.65799
Leaf 6 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 7 Corr. Reading	153.7497	155.1491	155.624	155.9356	156.0408	155.6861	154.2019
Leaf 7 Deviation(%)	-0.93329	-0.031611	0.27438	0.47513	0.54293	0.31439	-0.64194
Leaf 7 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 8 Corr. Reading	153.772	155.1242	155.6342	155.9575	155.9987	155.6836	154.2923
Leaf 8 Deviation(%)	-0.9258	-0.05457	0.27397	0.4823	0.50887	0.30583	-0.59059
Leaf 8 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 9 Corr. Reading	153.8892	155.1513	155.5266	155.837	156.0598	155.7974	154.3678
Leaf 9 Deviation(%)	-0.86551	-0.052464	0.1893	0.38927	0.5328	0.36377	-0.55717
Leaf 9 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 10 Corr. Reading	153.812	155.0102	155.5026	155.8316	155.9671	155.8207	154.4393
Leaf 10 Deviation(%)	-0.89285	-0.12075	0.19653	0.40851	0.49578	0.40144	-0.48865
Leaf 10 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 11 Corr. Reading	153.7832	154.9252	155.4894	155.8442	155.8779	155.7494	154.4477
Leaf 11 Deviation(%)	-0.88708	-0.15104	0.21255	0.44122	0.463	0.38013	-0.45878
Leaf 11 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 12 Corr. Reading	153.6698	154.8309	155.3785	155.7321	155.8243	155.7297	154.3519
Leaf 12 Deviation(%)	-0.90542	-0.15668	0.19641	0.42448	0.48389	0.42289	-0.46556
Leaf 12 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 13 Corr. Reading	153.6304	154.8373	155.4252	155.76	155.8001	155.6681	154.3351
Leaf 13 Deviation(%)	-0.92528	-0.14696	0.23221	0.44807	0.47397	0.38884	-0.47085
Leaf 13 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 14 Corr. Reading	153.5289	154.7991	155.3977	155.7315	155.7366	155.5754	154.3458
Leaf 14 Deviation(%)	-0.95958	-0.14019	0.24592	0.46126	0.46459	0.36062	-0.43263
Leaf 14 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 15 Corr. Reading	153.4723	154.7931	155.3134	155.687	155.7584	155.5036	154.3958
Leaf 15 Deviation(%)	-0.97862	-0.12643	0.20926	0.45026	0.49637	0.33198	-0.38282
Leaf 15 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 16 Corr. Reading	153.5108	154.8016	155.152	155.5457	155.8136	155.5129	154.4259
Leaf 16 Deviation(%)	-0.93911	-0.10613	0.11995	0.37403	0.54693	0.35288	-0.34855
Leaf 16 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 17 Corr. Reading	153.5355	154.8177	155.1238	155.4756	155.8014	155.5027	154.4331
Leaf 17 Deviation(%)	-0.91653	-0.089043	0.10847	0.33552	0.54577	0.35303	-0.33722
Leaf 17 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 18 Corr. Reading	153.5438	154.8255	155.1115	155.5086	155.8507	155.5587	154.4927
Leaf 18 Deviation(%)	-0.92958	-0.10259	0.081919	0.33814	0.55888	0.37053	-0.31729
Leaf 18 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 19 Corr. Reading	153.6092	154.8476	155.075	155.4779	155.8684	155.6077	154.5305
Leaf 19 Deviation(%)	-0.89879	-0.099799	0.046875	0.30683	0.55876	0.39052	-0.30439
Leaf 19 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 20 Corr. Reading	153.683	154.9087	155.0107	155.4399	155.8932	155.6439	154.6014
Leaf 20 Deviation(%)	-0.86618	-0.075544	-0.0097846	0.26708	0.55952	0.39871	-0.27381
Leaf 20 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 21 Corr. Reading	153.7286	154.9614	155.0635	155.4998	155.9669	155.7647	154.7013
Leaf 21 Deviation(%)	-0.88296	-0.088061	-0.02228	0.25907	0.5602	0.42983	-0.25579
Leaf 21 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 22 Corr. Reading	153.8619	155.0688	155.2836	155.6727	156.0793	155.8531	154.8475
Leaf 22 Deviation(%)	-0.8865	-0.10908	0.029265	0.27997	0.54183	0.39614	-0.25163




The RIT Family of Products

RADIOLOGICAL IMAGING TECHNOLOGY, INC.

	F1	F2	F3	F4	F5	F6	F7
Leaf 22 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 23 Corr. Reading	153.9913	155.1997	155.4401	155.8233	156.1825	155.9376	154.9373
Leaf 23 Deviation(%)	-0.88021	-0.10242	0.052295	0.29895	0.53016	0.37254	-0.27133
Leaf 23 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 24 Corr. Reading	154.1312	155.3328	155.609	155.9432	156.2773	156.0406	155.0834
Leaf 24 Deviation(%)	-0.87277	-0.09994	0.077661	0.29264	0.50746	0.35528	-0.26033
Leaf 24 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 25 Corr. Reading	154.2135	155.4345	155.7392	156.119	156.3602	156.1294	155.1726
Leaf 25 Deviation(%)	-0.8882	-0.10347	0.092345	0.33648	0.49146	0.34316	-0.27179
Leaf 25 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 26 Corr. Reading	154.3526	155.5484	156.0027	156.3685	156.4195	156.2223	155.2739
Leaf 26 Deviation(%)	-0.89155	-0.12374	0.16797	0.4028	0.43557	0.30893	-0.29999
Leaf 26 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 27 Corr. Reading	154.509	155.6379	156.1638	156.5135	156.5379	156.433	155.3856
Leaf 27 Deviation(%)	-0.88141	-0.15719	0.18017	0.40452	0.42015	0.35284	-0.31908
Leaf 27 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 28 Corr. Reading	154.7113	155.7796	156.281	156.616	156.6627	156.5775	155.4074
Leaf 28 Deviation(%)	-0.82932	-0.14456	0.17689	0.39159	0.42155	0.36694	-0.3831
Leaf 28 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 29 Corr. Reading	154.881	155.8898	156.324	156.6449	156.7491	156.7128	155.5052
Leaf 29 Deviation(%)	-0.78153	-0.1353	0.14289	0.34843	0.41521	0.39195	-0.38166
Leaf 29 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 30 Corr. Reading	155.0152	156.034	156.4973	156.8367	156.8715	156.8129	155.6677
Leaf 30 Deviation(%)	-0.78891	-0.13688	0.15961	0.37683	0.39909	0.3616	-0.37135
Leaf 30 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 31 Corr. Reading	155.1853	156.2442	156.6335	156.9487	157.0745	156.9758	155.7783
Leaf 31 Deviation(%)	-0.78031	-0.1033	0.14559	0.34714	0.42758	0.36448	-0.40117
Leaf 31 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 32 Corr. Reading	155.3558	156.4954	156.7941	157.1201	157.3189	157.0748	155.7886
Leaf 32 Deviation(%)	-0.77171	-0.043775	0.14702	0.35519	0.48218	0.32631	-0.49522
Leaf 32 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 33 Corr. Reading	155.3833	156.5764	157.0471	157.3625	157.3565	157.0519	155.8096
Leaf 33 Deviation(%)	-0.81198	-0.05039	0.25009	0.45143	0.44759	0.25312	-0.53986
Leaf 33 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 34 Corr. Reading	155.4608	156.7423	157.1701	157.4482	157.5285	157.1473	155.8028
Leaf 34 Deviation(%)	-0.82698	-0.0094804	0.26344	0.44085	0.49204	0.24891	-0.60878
Leaf 34 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 35 Corr. Reading	155.541	156.6896	157.23	157.5233	157.4118	157.1503	155.7794
Leaf 35 Deviation(%)	-0.77808	-0.045422	0.29932	0.48642	0.41534	0.24848	-0.62605
Leaf 35 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 36 Corr. Reading	155.4511	156.6892	157.1706	157.4629	157.4247	157.0473	155.8015
Leaf 36 Deviation(%)	-0.81032	-0.020319	0.28687	0.47333	0.44896	0.20819	-0.58671
Leaf 36 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 37 Corr. Reading	155.3303	156.6683	157.0823	157.3583	157.3589	156.8805	155.6766
Leaf 37 Deviation(%)	-0.82485	0.029452	0.29378	0.47004	0.47038	0.16492	-0.60372
Leaf 37 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 38 Corr. Reading	155.1802	156.4382	157.0049	157.2803	157.1011	156.6812	155.5892
Leaf 38 Deviation(%)	-0.82295	-0.018948	0.34323	0.5192	0.40471	0.13635	-0.56159
Leaf 38 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 39 Corr. Reading	154.958	156.0819	156.5467	156.8169	156.6963	156.3718	155.3223
Leaf 39 Deviation(%)	-0.74014	-0.020188	0.27755	0.45064	0.37337	0.1655	-0.50674
Leaf 39 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass
Leaf 40 Corr. Reading	154.4556	155.4955	155.9456	156.1974	156.0831	155.7594	154.7876
Leaf 40 Deviation(%)	-0.69208	-0.023471	0.2659	0.42779	0.35434	0.14616	-0.47864
Leaf 40 Pass/Fail	Pass	Pass	Pass	Pass	Pass	Pass	Pass



Horizontal Normalized Profiles

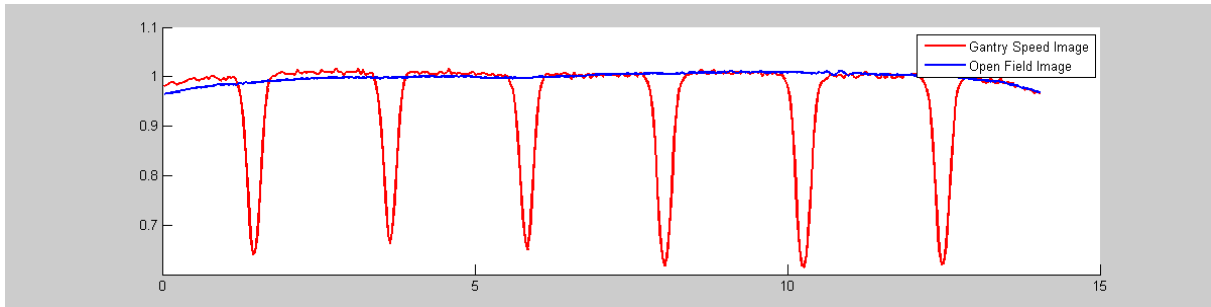

Settings

SID	100 cm
Delta X	5 pixels
Delta Y	10 pixels
Difference Tolerance	2%