

## ACR Small MR Phantom - Localizer Report


### OVERALL RESULTS

 ALL TOLERANCES PASSING	 ANALYSIS COMPLETE
---	--

### Image Information

Filename	C:\RIT\RIT113V4\demo images_old\Radia Demo Images\ACR_MRI_Small\Small_Localizer
Institution	Community Medical Center
Station	lx-mrcmc
Magnetic Field Strength	1.5
Protocol	PHYSICS ACR/
DICOM Slice Thickness(mm)	20
SOP Instance UID	1.2.840.113619.2.134.1762880825.2225.1250856598.501
Slice Location	-0.58537
Echo Time	20
Repetition Time	200
In Plane Phase Encoding Direction	ROW
Pixel Bandwidth	122.1094
ReceiveCoilName	LGEXTPA
Transmit Coil Name	
Flip Angle	90
Device Serial Number	000000000000234
Software Version	09
Scan Options	SAT_GEMS\\VB_GEMS \\SP
Echo Number	1
Echo Train Length	0
Operating Mode	

### Analysis Image

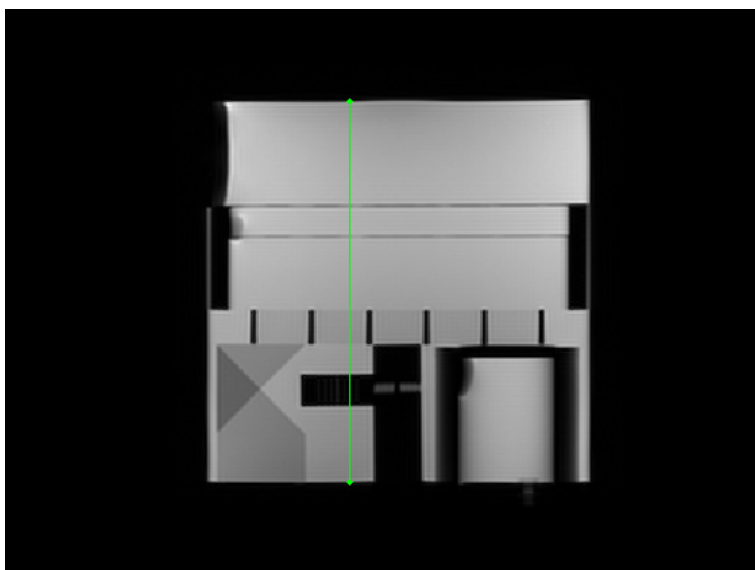

## Localizer Line Length

Localizer Line Length (mm)	99.53
ACR Minimum (mm)	99.00
ACR Maximum (mm)	103.00
Pass-Fail	Pass

## Analysis Settings

Localizer Phantom Threshold (Small)	0.5
Localizer Phantom Flipped LR	0