

Varian Dynamic MLC Test 6 (Pyramid)

Varian MLC Pyramid Image


Aligned Image

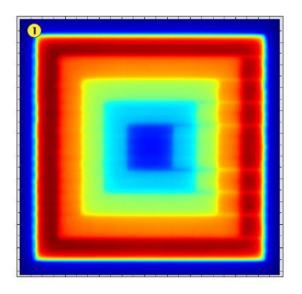


Uniformity

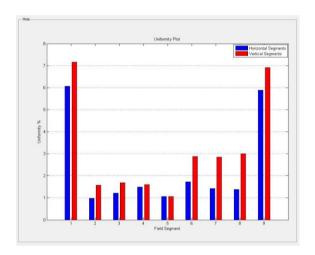


FWHM

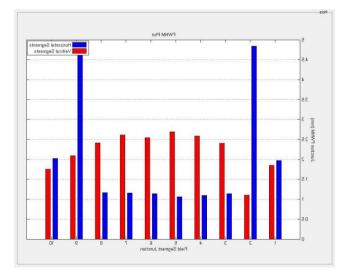

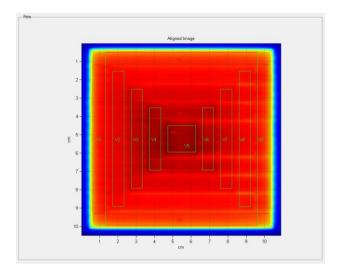

Position

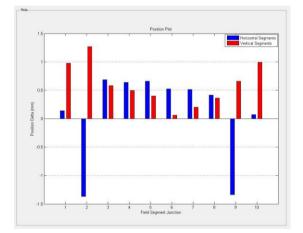

RIT113 Pyramid Analysis										
File Name:	C:\RIT\RIT113V4\Demo Images\MLC\Tests\edr2_test6_a-b.rv4									
SSD (cm):	100									
POSITION										
Area:	1	2	3	4	5	6	7	8	9	10
Tolerance:	1	1	1	1	1	1	1	1	1	1
Pos. Delta Horizontal:	0.14	-1.37	0.68	0.64	0.66	0.53	0.52	0.41	-1.33	0.07
Pass-Fail Horizontal:	Pass	Fail	Pass	Pass	Pass	Pass	Pass	Pass	Fail	Pass
Pos. Delta Vertical:	0.98	1.27	0.58	0.5	0.4	0.06	0.2	0.36	0.66	0.99
Pass-Fail Vertical:	Pass	Fail	Pass	Pass						
UNIFORMITY										
Area:	1	2	3	4	5	6	7	8	9	
Tolerance:	10	10	10	10	10	10	10	10	10	
Uniformity:	6.06	0.97	1.21	1.49	1.06	1.72	1.42	1.39	5.88	
Pass-Fail Horizontal:	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	
Uniformity:	7.16	1.58	1.68	1.61	1.06	2.88	2.85	3	6.91	
Pass-Fail Vertical:	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	
FWHM										
Area:	1	2	3	4	5	6	7	8	9	10
Tolerance:	3	3	3	3	3	3	3	3	3	3
FWHM Horizontal:	1.97	4.84	1.14	1.1	1.06	1.14	1.16	1.17	4.61	2.03
Pass-Fail Horizontal:	Pass	Fail	Pass	Pass	Pass	Pass	Pass	Pass	Fail	Pass
FWHM Vertical:	1.85	1.1	2.41	2.59	2.69	2.55	2.61	2.42	2.09	1.76
Pass-Fail Vertical:	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass

Summary Report